

# Lubricating Oil Analysis by Benchtop WDXRF According to ASTM D6443-04

**Application**

lubricating oil

**Instrument**Benchtop wavelength dispersive  
X-ray fluorescence spectrometer  
**Supermini200****Keywords**lubricating oil  
lube oil  
lubricant  
lubricant additives  
oil  
petrochemical  
ASTM  
D6443-04  
benchtop**Introduction**

Lubricating oils are given specific functional properties by mixing additives with base oil. In order to assure consistent and desirable performance, it is very important to control the concentrations of the additives during the lubricant manufacturing process.

X-ray fluorescence (XRF) spectrometry has become increasingly popular for quantitative elemental analysis of base oils as well as additives and lubricant products due to its high precision and simple sample preparation. With liquids, sample preparation for XRF typically means simply pouring the sample into a plastic cup with a transparent film. Unlike other techniques, such as Inductively-Coupled Plasma Optical Emission Spectroscopy (ICP-OES), XRF does not require time-consuming processes such as chemical decomposition, digestion or serial dilution. ASTM D6443-04 specifies the use of the wavelength-dispersive (WD) XRF technique since it offers sufficiently high precision, resolution and light-element sensitivity to meet the industry's needs.

Traditionally, WDXRF spectrometers have been large floor-standing models with substantial installation requirements and high replacement cost of faulty components. In its search for greater cost-efficiency, the lubricant industry is turning to tools that not only do the job, but are also easier and less costly to acquire,

install and maintain.

This application note demonstrates the capability of low-cost, compact benchtop WDXRF spectrometer for quantitative elemental analysis of Ca, Cl, Cu, Mg, P, S and Zn in base oils, lubricating oils and additives according to ASTM D6443-04.

**Instrument**

The Supermini200 is a benchtop sequential WDXRF spectrometer designed specifically to deliver excellent performance while eliminating typical installation requirements such as cooling water, special power supply, large floor space.

Featuring a unique air-cooled 200W X-ray tube, two detectors, programmable vacuum or helium environment, and three analyzing crystals, the Supermini200 can analyze all relevant elements in just a few minutes with full spectral separation of all peaks and excellent sensitivity for light elements such as Mg, P and Cl.

The Windows®-based software used to operate the Supermini200 is shares the same platform running Rigaku's popular higher-power WDXRF ZSX family instruments. This means that it has the same advanced algorithms, multiple language support and an intuitive user-friendly interface that have made Rigaku the world's leader in X-ray instrumentation and industrial applications.

## Standards and Sample Preparation

Organometallic reference standard samples for lubricating oil provided by AccuStandard®, Inc. were used as calibration standards.

Six grams of each sample was poured into a liquid cell (Chemplex® 1540) with 4.0 µm Prolene® (Chemplex® 416) as sample film. The cups are disposable and inexpensive.

## Measurement Conditions

All elements were measured in helium atmosphere, using standard crystals, with the X-ray tube operating at 50 kV and 4.0 mA. Peak and background intensities were counted for each element line, and the total counting time was less than nine minutes.

## Calibration

In accordance with ASTM D6443-04, empirical matrix corrections were applied for all analytes except Mg. The calibration results are listed in Table 1, with the corresponding calibration curves shown in Figure 1.

**Table 1** Calibration results for all elements

Element	Calibration Range (mass%)	Accuracy (mass%)	LLD (ppm)
Ca	0 – 0.50	0.0021	1.9
Cl	0 – 0.15	0.0005	0.8
Cu	0 – 0.05	0.0006	1.1
Mg	0 – 0.20	0.0044	20
P	0 – 0.15	0.0004	1.0
S	0 – 0.75	0.0032	0.9
Zn	0 – 0.15	0.0020	1.0

The calibration accuracy was calculated by the following formula,

$$\text{Accuracy} = \sqrt{\frac{\sum_i (C_i - \hat{C}_i)^2}{n - 2}}$$

$\hat{C}_i$  : reference value of standard sample

n : number of standard samples.

The lower limit of detection (LLD) was calculated as follows;

$$\text{LLD} = 3 \cdot \frac{1}{m} \cdot \sigma_B = \frac{3}{m} \cdot \sqrt{\frac{I_B}{1000 \times t}}$$

m : sensitivity of calibration (kcps/ppm)

$\sigma_B$  : standard deviation of blank intensity (kcps)


$I_B$  : blank intensity (kcps)

t : counting time (s).

## Analysis results

To confirm that the spectrometer's repeatability performance is compliant with the requirement of the method, two aliquots of a representative sample were prepared and quantified. This process was repeated twenty times.

The test data compiled in Table 2 shows the average and the difference between the two-aliquot measurement results. ASTM D6443-04 specifies that "the difference between successive test results obtained by

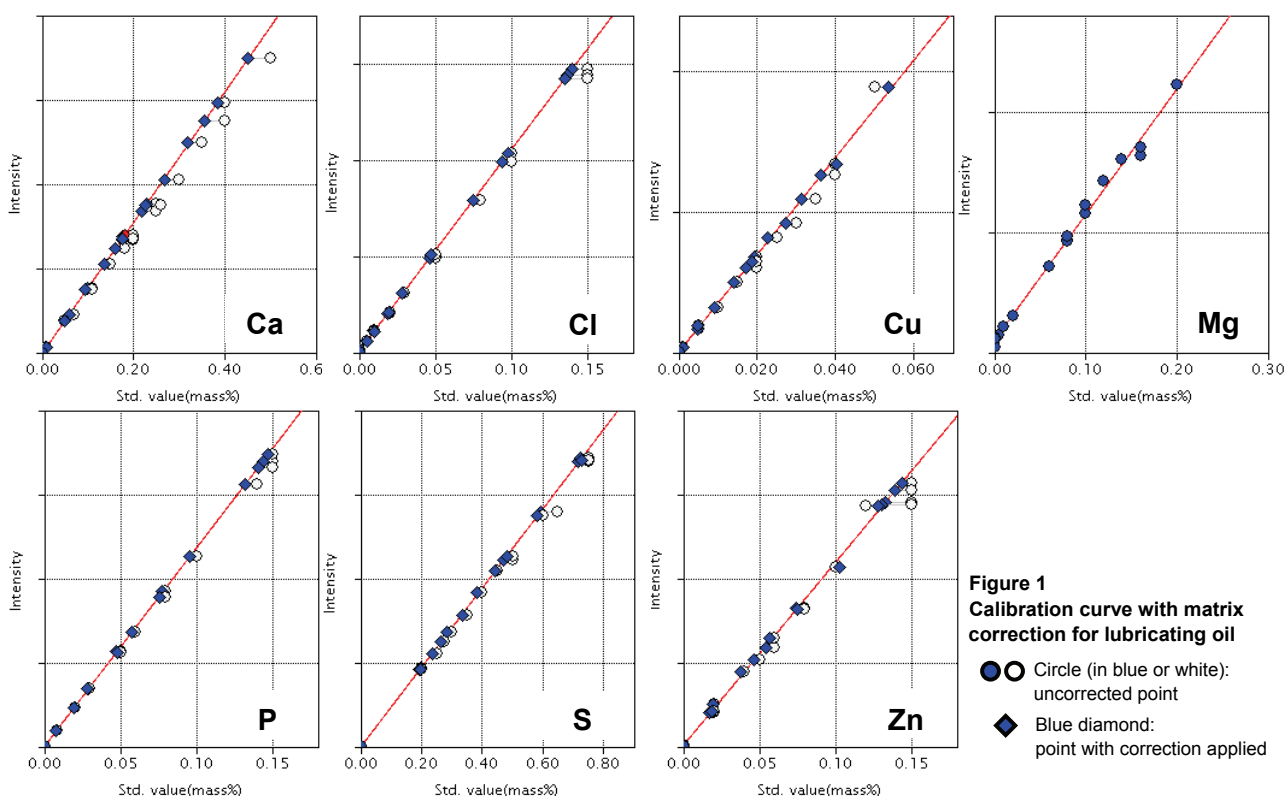

the same operator with the same apparatus under constant operation conditions on identical test material...in the long run” must not exceed the values in Table 3, which shows the formula for the maximum allowed repeatability “*r*” of each analyte. All units in Table 3 are in terms of mass%, including the standards’ concentration.

“Max” indicated in Table 2 is the maximum actual obtained difference between successive results, while “*r*” represents the maximum permissible difference as prescribed by the ASTM method (see Table 3). Since “Max” never exceeds “*r*”, the repeatability performance of the Supermini200 easily satisfies the requirements of ASTM D6443-04.

Table 2 Repeatability test results

(unit: mass%)

	Ca		Cl		Cu		Mg	
	Avg.	Diff.	Avg.	Diff.	Avg.	Diff.	Avg.	Diff.
1	0.0102	0.0001	0.0107	0.0000	0.0118	0.0002	0.0332	0.0020
2	0.0102	0.0001	0.0106	0.0002	0.0118	0.0001	0.0324	0.0004
3	0.0102	0.0000	0.0106	0.0001	0.0119	0.0001	0.0326	0.0000
4	0.0103	0.0001	0.0106	0.0000	0.0118	0.0002	0.0340	0.0027
5	0.0103	0.0001	0.0105	0.0002	0.0117	0.0000	0.0351	0.0005
6	0.0102	0.0000	0.0105	0.0002	0.0118	0.0002	0.0332	0.0033
7	0.0103	0.0002	0.0107	0.0001	0.0120	0.0001	0.0337	0.0044
8	0.0104	0.0001	0.0107	0.0000	0.0118	0.0004	0.0340	0.0039
9	0.0103	0.0001	0.0107	0.0000	0.0117	0.0001	0.0342	0.0043
10	0.0102	0.0001	0.0107	0.0001	0.0118	0.0001	0.0338	0.0050
11	0.0103	0.0003	0.0106	0.0001	0.0119	0.0002	0.0331	0.0035
12	0.0105	0.0001	0.0106	0.0001	0.0120	0.0000	0.0353	0.0009
13	0.0104	0.0002	0.0106	0.0001	0.0119	0.0002	0.0341	0.0032
14	0.0102	0.0003	0.0106	0.0001	0.0118	0.0001	0.0338	0.0025
15	0.0102	0.0003	0.0106	0.0001	0.0117	0.0000	0.0342	0.0016
16	0.0103	0.0000	0.0105	0.0000	0.0118	0.0001	0.0338	0.0008
17	0.0104	0.0002	0.0106	0.0001	0.0118	0.0000	0.0340	0.0005
18	0.0104	0.0002	0.0105	0.0003	0.0118	0.0001	0.0333	0.0009
19	0.0102	0.0002	0.0104	0.0001	0.0118	0.0002	0.0338	0.0019
20	0.0100	0.0003	0.0105	0.0001	0.0118	0.0002	0.0339	0.0016
<b>Max</b>		<b>0.0003</b>		<b>0.0003</b>		<b>0.0004</b>		<b>0.0050</b>
<b>r</b>		<b>0.0007</b>		<b>0.0007</b>		<b>0.0004</b>		<b>0.0053</b>
	P		S		Zn			
	Avg.	Diff.	Avg.	Diff.	Avg.	Diff.		
1	0.0100	0.0001	0.0474	0.0003	0.0113	0.0000		
2	0.0100	0.0001	0.0476	0.0001	0.0114	0.0001		
3	0.0100	0.0001	0.0477	0.0002	0.0115	0.0001		
4	0.0100	0.0000	0.0476	0.0005	0.0114	0.0002		
5	0.0101	0.0001	0.0474	0.0002	0.0113	0.0001		
6	0.0100	0.0003	0.0477	0.0003	0.0114	0.0003		
7	0.0098	0.0000	0.0478	0.0000	0.0115	0.0001		
8	0.0100	0.0003	0.0476	0.0005	0.0114	0.0001		
9	0.0102	0.0002	0.0477	0.0007	0.0113	0.0000		
10	0.0102	0.0003	0.0479	0.0002	0.0113	0.0000		
11	0.0101	0.0001	0.0479	0.0001	0.0114	0.0002		
12	0.0102	0.0001	0.0478	0.0002	0.0115	0.0000		
13	0.0101	0.0002	0.0477	0.0001	0.0115	0.0000		
14	0.0100	0.0000	0.0478	0.0003	0.0115	0.0000		
15	0.0099	0.0002	0.0477	0.0004	0.0116	0.0001		
16	0.0099	0.0002	0.0474	0.0003	0.0115	0.0002		
17	0.0100	0.0001	0.0474	0.0003	0.0114	0.0001		
18	0.0101	0.0003	0.0474	0.0002	0.0114	0.0001		
19	0.0100	0.0004	0.0474	0.0002	0.0114	0.0000		
20	0.0098	0.0000	0.0474	0.0002	0.0114	0.0000		
<b>Max</b>		<b>0.0004</b>		<b>0.0007</b>		<b>0.0003</b>		
<b>r</b>		<b>0.0008</b>		<b>0.0015</b>		<b>0.0005</b>		

**Table 3 Repeatability as defined in ASTM D6443-04** (unit: mass%)

Element	Concentration range	Repeatability [r]
Ca	0.001 – 0.200	0.006914 (X+0.0007) <sup>0.5</sup>
Cl	0.001 – 0.030	0.0356 (X+0.0086)
Cu	0.001 – 0.030	0.002267 (X+0.0013) <sup>0.4</sup>
Mg	0.003 – 0.200	0.01611 (X+0.0008) <sup>0.333</sup>
P	0.001 – 0.200	0.02114 X <sup>0.7</sup>
S	0.030 – 0.800	0.02371 X <sup>0.9</sup>
Zn	0.001 – 0.200	0.01225 X <sup>0.7</sup>

Note) X: concentration in mass%

Qualitative scans of each analyte element are shown in Figure 2 which demonstrates the excellent peak-to-background ratio and spectral resolution of the wavelength-dispersive technology in the Rigaku Supermini200.


## Conclusions

This application note demonstrates that lubricating oils and additives can be routinely analyzed with excellent accuracy, sensitivity and repeatability using a benchtop WDXRF spectrometer with minimal installation requirements.

In particular, the Rigaku Supermini200 sequential WDXRF spectrometer meets the specifications of ASTM D6443-04, as well as those of ASTM D4927-05, which applies to higher concentrations of additive elements.

## Reference

ASTM D6443-04 (2010) Standard Test Method for Determination of Calcium, Chlorine, Copper, Magnesium, Phosphorus, Sulfur, and Zinc in Unused Lubricating Oils and Additives by Wavelength Dispersive X-ray Fluorescence Spectrometry (Mathematical Correction Procedure)

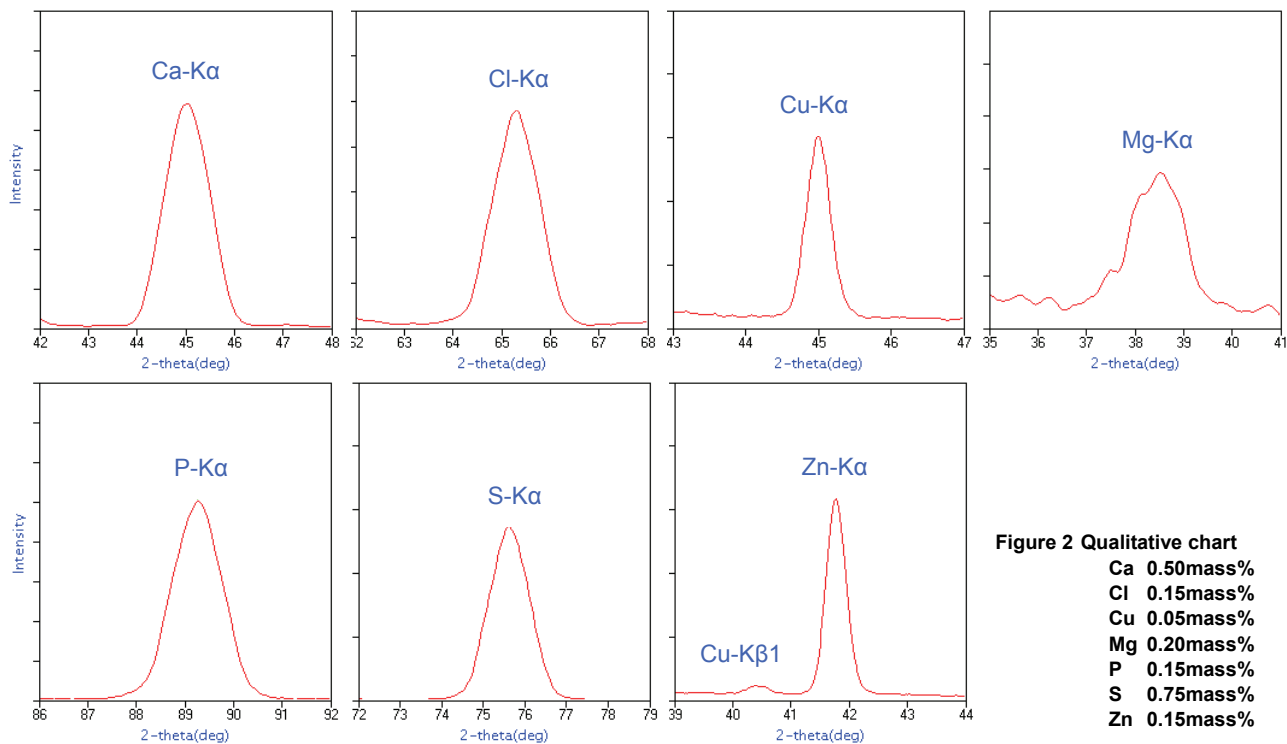

**Rigaku Corporation** Tokyo Branch  
4-14-4, Sendagaya, Shibuya-ku, Tokyo 151-0051, Japan  
Phone +81-3-3479-0618 Fax +81-3-3479-6112 rinttyo@rigaku.co.jp

[www.Rigaku.com](http://www.Rigaku.com)

**Rigaku Corporation**  
Head Office  
3-9-12, Matsubara-cho, Akishima-shi, Tokyo 196-8666, Japan  
Phone +81-42-545-8189 Fax +81-42-544-9223  
rinttyo@rigaku.co.jp

**Rigaku Americas Corporation**  
9009 New Trails Drive, The Woodlands, Texas 77381-5209, USA  
Phone +1-281-362-2300 Fax +1-281-364-3628  
info@rigaku.com

**Rigaku Europe SE**  
Am Hardtward 11, 76275 Ettlingen, Germany  
Phone +49-7243-94936-0 Fax +49-7243-94936-10  
rese@rigaku.com

**Rigaku Corporation**  
Osaka Factory  
14-8, Akaoji-cho, Takatsuki-shi, Osaka 569-1146, Japan  
Phone +81-72-693-7990 Fax +81-72-693-6746  
rinttyo@rigaku.co.jp

**Rigaku Beijing Corporation**  
2601A, Tengda Plaza, No.168, Xizhimenwai Avenue,  
Haidian District, Beijing 100044, P.R.China  
Phone +86-010-8857-5768 Fax +86-010-8857-5748  
info@rigaku.com.cn

**Rigaku Latin America Ltda.**  
Rua Harmonia, 1232, Sumarezinho,  
CEP 05435-001, São Paulo, SP, Brazil  
Phone +55-11-4999-0756 Fax +55-11-4999-0756  
rinttyo@rigaku.co.jp

(L0523en)